



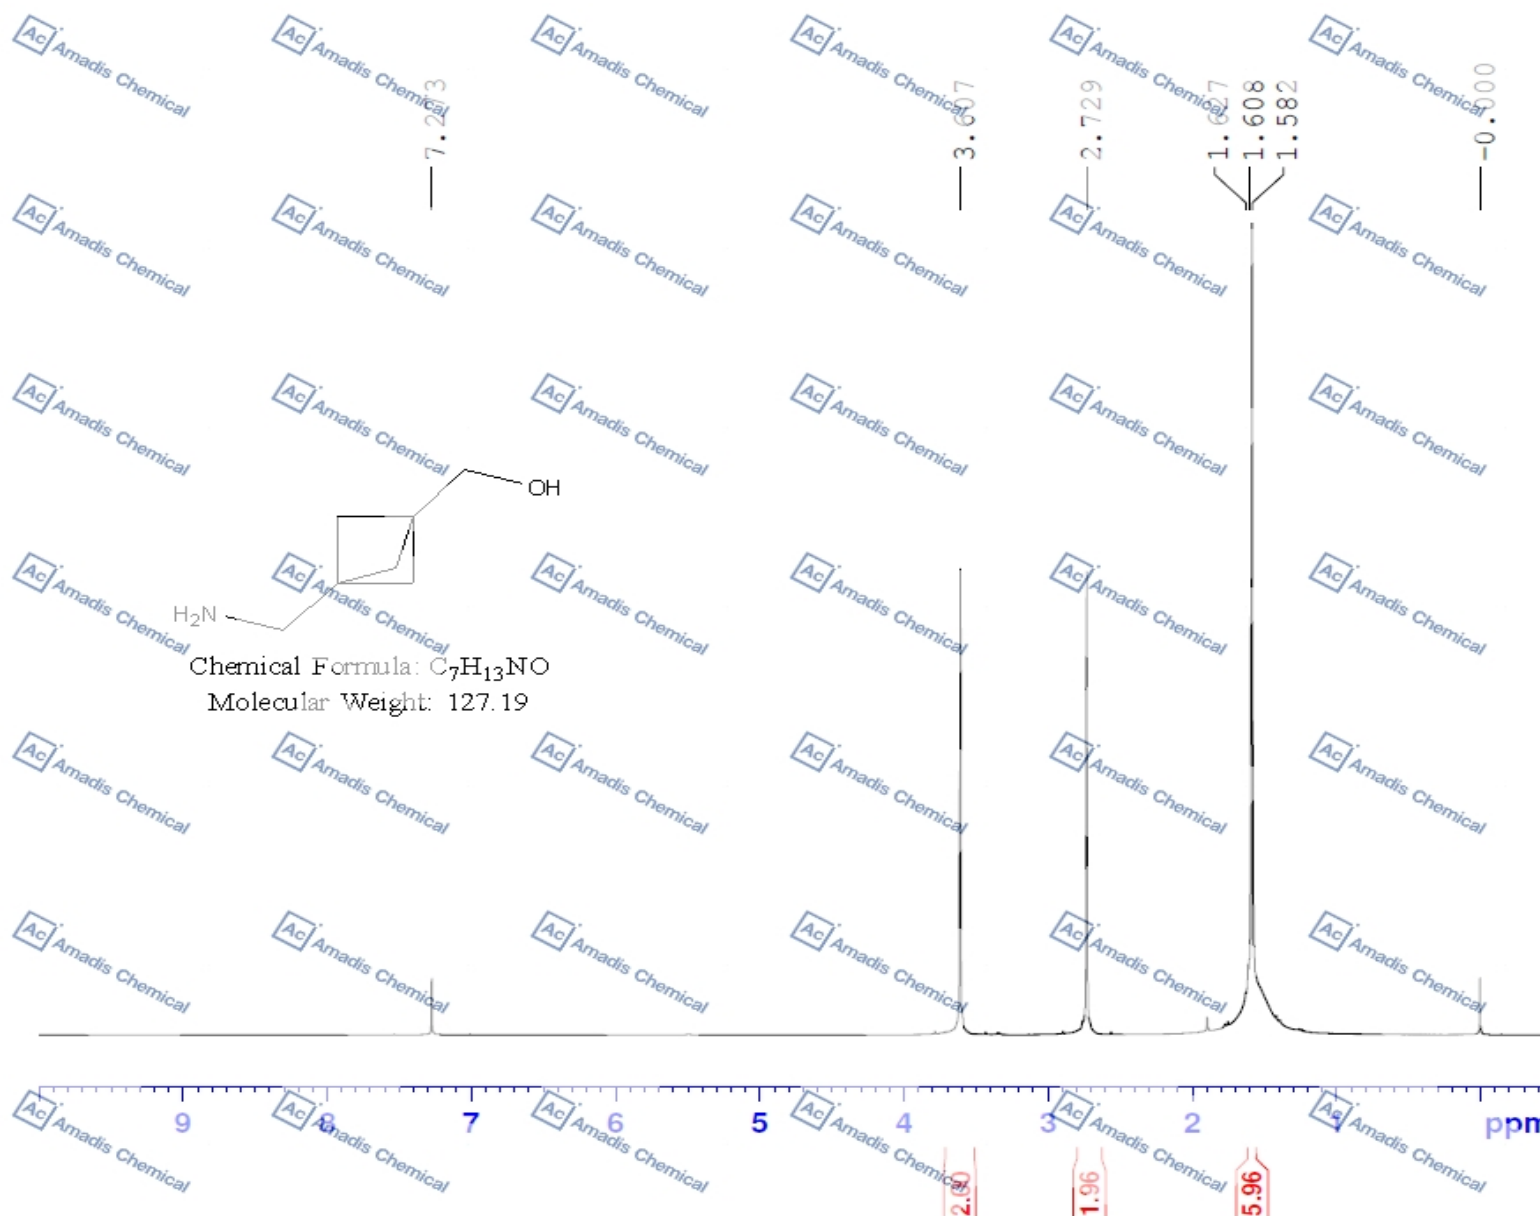

Current Data Parameters  
 Name: 0621-10  
 EXPNO: 10  
 PROCNO: 1

F2 - Acquisition Parameters  
 Date\_ 20240624  
 Time 13.46 h  
 INSTRUM spect  
 P1 4.09  
 P2 2.9  
 TD 65536  
 SOLVENT CDCl3  
 NS 16  
 DS 2  
 SWH 8012.820 Hz  
 FIDRES 0.244532 Hz  
 ACQ 4.089465 sec  
 R 8.000000 sec  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 299.3 K  
 D1 1.00000000 sec  
 TD0 1  
 SFO1 400.1524709 MHz  
 NUC1 1H  
 P1 10.00 usec  
 P2 14.6979949 usec

F2 - Processing parameters  
 SI 65536  
 SF 400.1500044 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

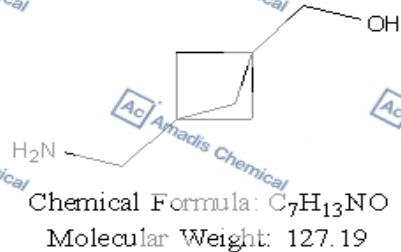

\*For laboratory or manufacturing use only, not for drug, food and household use.